

Keysight Signal Generators

This manual provides documentation for the following instruments:

MXG Signal Generator (Series A)

ESG Signal Generator

Security
Features and
Document of
Volatility

Notices

Copyright Notice

© Keysight Technologies 2004-2017

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies, Inc. as governed by United States and international copyright laws.

Manual Part Number

E4400-90621

Edition

Edition 3, October 2017

Supersedes: May 2017

Published by:

Keysight Technologies Inc.
1400 Fountaingrove Parkway
Santa Rosa, CA 95403

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

U.S. Government Rights

The Software is “commercial computer software,” as defined by Federal Acquisition Regulation (“FAR”) 2.101. Pursuant to FAR 12.212 and 27.405-3 and Department of Defense FAR Supplement (“DFARS”) 227.7202, the U.S. government acquires commercial computer software under the same terms by which the software is customarily provided to the public. Accordingly, Keysight provides the Software to U.S. government customers under its standard commercial license, which is embodied in its End User License Agreement (EULA), a copy of which can be found at

<http://www.keysight.com/find/sweula>

The license set forth in the EULA represents the exclusive authority by which the U.S. government may use, modify, distribute, or disclose the Software. The EULA and the license set forth therein, does not require or permit, among other things, that Keysight: (1) Furnish technical information related to commercial computer software or commercial computer software documentation that is not customarily provided to the public; or (2) Relinquish to, or otherwise provide, the government rights in excess of these rights customarily provided to the public to use, modify, reproduce, release, perform, display, or disclose commercial computer software or commercial computer software documentation. No additional government requirements beyond those set forth in the EULA shall apply, except to the extent that those terms, rights, or licenses are explicitly required from all providers of commercial computer software pursuant to the FAR and the DFARS and are set forth specifically in writing elsewhere in the EULA. Keysight shall be under no obligation to update, revise or otherwise modify the Software. With respect to any technical data as defined by FAR 2.101, pursuant to FAR 12.211 and 27.404.2 and DFARS 227.7102, the U.S. government acquires no greater than Limited Rights as defined in FAR 27.401 or DFAR 227.7103-5 (c), as applicable in any technical data.

Warranty

THE MATERIAL CONTAINED IN THIS DOCUMENT IS PROVIDED “AS IS,” AND IS SUBJECT TO BEING CHANGED, WITHOUT NOTICE, IN FUTURE EDITIONS. FURTHER, TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, KEYSIGHT DISCLAIMS ALL WARRANTIES, EITHER EXPRESS OR IMPLIED, WITH REGARD TO THIS MANUAL AND ANY INFORMATION CONTAINED HEREIN, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. KEYSIGHT SHALL NOT BE LIABLE FOR ERRORS OR FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH THE FURNISHING, USE, OR PERFORMANCE OF THIS DOCUMENT OR OF ANY INFORMATION CONTAINED HEREIN. SHOULD KEYSIGHT AND THE USER HAVE A SEPARATE WRITTEN AGREEMENT WITH WARRANTY TERMS COVERING THE MATERIAL IN THIS DOCUMENT THAT CONFLICT WITH THESE TERMS, THE WARRANTY TERMS IN THE SEPARATE AGREEMENT SHALL CONTROL.

Safety Information

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

Where to Find the Latest Information

Documentation is updated periodically. For the latest information about these products, including instrument software upgrades, application information, and product information, see one of the following URLs, depending on the model number of your instrument:

<http://www.keysight.com/find/mxg>

<http://www.keysight.com/find/esg>

To receive the latest updates by email, subscribe to Keysight Email Updates:

<http://www.keysight.com/find/emailupdates>

Information on preventing instrument damage can be found at:

<http://www.keysight.com/find/PreventingInstrumentRepair>

Is your product software up-to-date?

Periodically, Keysight releases software updates to fix known defects and incorporate product enhancements. To search for software updates for your product, go to the Keysight Technical Support website at:

<http://www.keysight.com/find/techsupport>

Table of Contents

| | | |
|---|--|----|
| 1 | Contacting Keysight Sales and Service Offices | 5 |
| 2 | Products Covered by this Document | 6 |
| | Document Purpose | 6 |
| | Recommended Software Upgrades | 7 |
| 3 | Security Terms and Definitions | 8 |
| 4 | Instrument Memory & Volatility | 9 |
| | MXG (Series A) Memory | 10 |
| | ESG Memory | 14 |
| 5 | Memory Clearing, Sanitization and Removal Procedures | 19 |
| | Erase All (Option 006 Only) | 20 |
| | Erase and Overwrite All | 21 |
| | Erase and Sanitize All (Option 006 Only) | 22 |
| | Clear Persistent State Information | 23 |
| | Instrument Setup | 23 |
| | LAN Setup (MXG Only) | 23 |
| | User IQ Cal File (Vector Models Only) | 23 |
| 6 | Using Secure Mode | 24 |
| 7 | Using Secure Display | 25 |
| 8 | Security Issues for Certain Firmware Revisions | 26 |
| | Firmware Update Procedure | 26 |
| | Error Messages and Secure Environments | 27 |
| | Recovering Erased System Files | 28 |
| 9 | Procedure for Declassifying a Faulty Instrument | 29 |
| | Appendix A References | 30 |

1 Contacting Keysight Sales and Service Offices

Assistance with test and measurement needs, and information to help you find a local Keysight office, is available via the internet at, <http://www.keysight.com/find/assist>. If you do not have internet access, please contact your designated Keysight representative.

NOTE

In any correspondence or telephone conversation, refer to the instrument by its model number and full serial number. With this information, the Keysight representative can determine whether your unit is still within its warranty period.

2 Products Covered by this Document

| Product Family Name | Product Name | Model Number | Firmware Revision |
|----------------------------|---------------------------------|---------------------|-------------------|
| X-Series Signal Generators | MXG Signal Generator (Series A) | N5183A | All |
| | | N5182A | |
| | | N5181A | |
| | | N5162A ^a | |
| | | N5161A ^a | |
| Keysight Signal Generators | ESG Signal Generator | E4438C ^b | C.03.40 or higher |
| | | E4428C ^b | All |

- a. For the N5161A/62A Signal Generators, the softkey menus and features described in this guide are only available through the web-enabled interface or via SCPI commands. Refer to the instrument [Installation Guide](#), [Programming Guide](#) and [SCPI Programmers Reference](#) for more information.
- b. See [“Recommended Software Upgrades” on page 7](#) for important firmware version information.

Document Purpose

This document describes instrument memory types and security features. It provides a statement regarding the volatility of all memory types, and specifies the steps required to declassify an instrument through memory clearing, sanitization, or removal.

For additional information, go to:

<http://www.keysight.com/find/security>

IMPORTANT

Be sure that all information stored by the user in the instrument that needs to be saved is properly backed up before attempting to clear any of the instrument memory. Keysight Technologies cannot be held responsible for any lost files or data resulting from the clearing of memory.

Be sure to read this document entirely before proceeding with any file deletion or memory clearing.

Recommended Software Upgrades

The information in this section applies only to **PSG** and **ESG** Signal Generators.

CAUTION

Do not use the **Erase All**, **Erase and Overwrite All**, **Erase and Sanitize All**, **Erase, Overwrite**, or **Sanitize** procedures with any of the firmware revisions listed in [Table 2-1](#) below.

If your instrument's current firmware revision is among those listed, please upgrade **immediately** to newer firmware. For details, see [“Firmware Update Procedure” on page 26](#).

Table 2-1 Firmware revisions that require upgrades

| Instrument model number | Current firmware revision | Upgrade to firmware revision |
|-------------------------|---------------------------|------------------------------|
| E44x8C | C.04.84, C.04.86, C.04.95 | C.04.96 or later |

3 Security Terms and Definitions

| Term | Definition |
|--------------------------------|---|
| Clearing | As defined in Section 8-301a of DoD 5220.22-M, “National Industrial Security Program Operating Manual (NISPOM)”, clearing is the process of eradicating the data on media before reusing the media in an environment that provides an acceptable level of protection for the data that was on the media before clearing. Hence, clearing is typically used when the instrument is to remain in an environment with an acceptable level of protection. |
| Instrument Declassification | A term that refers to procedures that must be undertaken before an instrument can be removed from a secure environment, such as is the case when the instrument is returned for calibration. Declassification procedures include memory sanitization or memory removal, or both. Keysight declassification procedures are designed to meet the requirements specified in DoD 5220.22-M, “National Industrial Security Program Operating Manual (NISPOM)”, Chapter 8. |
| Sanitization | <p>As defined in Section 8-301b of DoD 5220.22-M, “National Industrial Security Program Operating Manual (NISPOM)”, sanitization is the process of removing the data from media before reusing the media in an environment that does not provide an acceptable level of protection for the data that was in the media before sanitizing. Hence, instrument sanitization is typically required when an instrument is moved from a secure to a non-secure environment, such as when it is returned to the factory for calibration.</p> <p>Keysight memory sanitization procedures are designed for customers who need to meet the requirements specified by the US Defense Security Service (DSS). These requirements are specified in the “Clearing and Sanitization Matrix” in Section 5.2.5.5.5 of the <i>ISFO Process Manual for the Certification and Accreditation of Classified Systems under the NISPOM</i>.</p> |
| Secure Erase | Secure Erase is a term that is used to refer to either the clearing or sanitization features of Keysight instruments. |

4 Instrument Memory & Volatility

This chapter contains information on the memory components in your instrument.

The tables provide details of the size of each memory component, its type, how it is used, its location, volatility, and the sanitization procedure.

The descriptions are divided by product type, as follows:

- [“MXG \(Series A\) Memory” on page 10](#)
- [“ESG Memory” on page 14](#)

MXG (Series A) Memory

The following tables describe each memory type used in the base instrument and optional baseband generator.

Table 4-1 Base Instrument (All models and options)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|-----------------------------------|-----------------------------------|---------------------------------|---|--|--|---|
| 1. Main Memory (DRAM) 32 MByte | Yes | No | Firmware operating memory | Operating system | CPU board, not battery backed. | Turn off instrument power. |
| 2. Main Memory (Flash) 8 MByte | Yes | Yes | Factory calibration/ configuration data User file system ^a , which includes flatness calibration, instrument states, and sweep lists | Firmware upgrades and user-saved data ^a | CPU board (same chip as firmware memory, but managed separately) | Because this memory chip contains 8 MB of user data (described here) and 8 MB of firmware memory, a full-chip erase is not desirable. User data areas are selectively and completely sanitized by the procedure “Erase and Sanitize All (Option 006 Only)” on page 22. |

Table 4-1 Base Instrument (All models and options)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|--|-----------------------------------|---------------------------------|---|--|---|---|
| 3. Firmware Memory (Flash) 8 MByte | No | Yes | Main firmware image | Factory installed or firmware upgrade During normal operation, this memory cannot be overwritten. | CPU board (same chip as main flash memory, but managed separately) | Because this memory chip contains 8 MB of user data and 8 MB of firmware memory (described here), a full-chip erase is not desirable. User data areas are selectively and completely sanitized by the procedure "Erase and Sanitize All (Option 006 Only)" on page 22. |
| 4. Bootrom Memory (EEPROM) 8 KByte | No | Yes | CPU bootup parameters | Factory programmed | CPU board | None required (no user data) |
| | Yes | Yes | LAN configuration | Front panel entry or remotely | During normal operation, this memory cannot be overwritten or erased except for LAN configuration. This read-only data is programmed at the factory. | |
| 5. Calibration Data (Flash) 256 KByte | No | Yes | Factory calibration and configuration data backup | Factory or service only | RF Board | None required (no user data) |

Table 4-1 Base Instrument (All models and options)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|---|-----------------------------------|---------------------------------|--|-------------------|------------------------------------|------------------------------|
| 6. LCD Display Memory (DRAM) 160 KByte | No | No | Display buffer | Operating system | CPU board, not battery backed. | Turn off instrument power. |
| 7. Front Panel Memory (Flash) 32 KByte | No | Yes | Front panel keyboard controller firmware | Operating system | Front Panel board | None required (no user data) |

a. Analog instruments only

Table 4-2 Vector Models with Baseband Generator (N5162A/N5182A with Options 651, 652, or 654)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|---|-----------------------------------|---------------------------------|--|-----------------------|------------------------------------|---|
| 1. Waveform Memory (DRAM) ≤ 320 MByte | Yes | No | Waveforms (including header and marker data) | Normal user operation | Not battery backed. | Turn off instrument power. |
| 2. Extended Persistent Memory (Flash) ^a 4 GByte | Yes | Yes | All user data | Normal user operation | | User data is completely sanitized by the procedure “Erase and Sanitize All (Option 006 Only)” on page 22. |

Instrument Memory & Volatility
 MXG (Series A) Memory

Table 4-2 Vector Models with Baseband Generator (N5162A/N5182A with Options 651, 652, or 654)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|---|-----------------------------------|---------------------------------|------------------|-------------------------|------------------------------------|------------------------------|
| 3. Calibration Data Memory (Flash) 128 KByte | No | Yes | No user data | Factory or service only | | None required (no user data) |

a. For serial numbers lower than MY/US/SG4818xxxx, the persistent memory value is 512 MByte.

ESG Memory

The following tables describe each memory type used in the base instrument, optional baseband generator, optional hard disk and option flash drive.

Table 4-3 Base Instrument (All models and options)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|------------------------------------|-----------------------------------|---------------------------------|---|---------------------------------------|--|---|
| 1. Main Memory (SDRAM) 64 MByte | Yes | No | Firmware operating memory | Operating system (not user) | CPU board. Not battery backed. | Turn off instrument power. |
| 2. Main Memory (Flash) 20 MByte | Yes | Yes | Factory calibration/ configuration data User file system, which includes instrument status backup, flatness calibration, IQ calibration, instrument states, waveforms (including header and marker data), modulation definitions, and sweep lists | Firmware upgrades and user-saved data | CPU board (same chip as firmware memory, but managed separately) User data is not stored in this memory if hard disk (Option 005) or flash drive (Option 008/009) is installed. | Because this 32 MB memory chip contains 20 MB of user data (described here) and 12 MB of firmware memory, a selective chip erase is performed. User data areas are selectively and completely sanitized by the procedure “Erase and Sanitize All (Option 006 Only)” on page 22. |

Table 4-3 Base Instrument (All models and options)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|---|-----------------------------------|---------------------------------|--|---------------------------------------|--|---|
| 3. Firmware Memory (Flash) 12 MByte | No | Yes | Main firmware image | Factory installed or firmware upgrade | CPU board (same chip as main flash memory, but managed separately) | Because this 32 MB memory chip contains 20 MB of user data and 12 MB of firmware memory (described here), a selective chip erase is performed. User data areas are selectively and completely sanitized by the procedure "Erase and Sanitize All (Option 006 Only)" on page 22. |
| | Yes | Yes | LAN configuration | Front panel entry or remotely | During normal operation, this memory cannot be overwritten except for LAN configuration. | |
| 4. Battery Backed Memory (SRAM) 512 KByte | Yes | Yes | User-editable data (table editors) Last instrument state, last instrument state backup, and persistent instrument state and instrument status | Firmware operations | CPU board The battery is located on the motherboard. | Sanitized by the procedure described in "Erase and Sanitize All (Option 006 Only)" on page 22. |
| 5. Bootrom Memory (Flash) 128 KByte | No | Yes | CPU bootup program and firmware loader/updater | Factory programmed | CPU board During normal operation, this memory cannot be overwritten or erased. | None required (no user data) |
| 6. Calibration Backup Memory (Flash) 512 KByte | No | Yes | Factory calibration/configuration data backup | Factory or service only | Motherboard | None required (no user data) |

Table 4-3 Base Instrument (All models and options)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|--|-----------------------------------|---------------------------------|--|------------------------------------|--|------------------------------|
| 7. Boards Memory (Flash) 512 Bytes | No | Yes | Factory calibration and information files, code images, and self-test limits | Factory or service only | All RF boards, baseband generator, and motherboard | None required (no user data) |
| 8. Micro-processor Cache (SRAM) 3 KByte | Yes | No | CPU data and instruction cache | Memory is managed by CPU, not user | CPU board, not battery backed. | Turn off instrument power. |

Table 4-4 Vector Models with Baseband Generator (E4438C with Options 601 or 602)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|--|-----------------------------------|---------------------------------|---|-----------------------|------------------------------------|---|
| 1. Waveform Memory (SDRAM) 40 MByte– 320 MByte | Yes | No | Waveforms (including header and marker data) and PRAM | Normal user operation | Not battery backed. | User data is completely sanitized by the procedure “Erase and Sanitize All (Option 006 Only)” on page 22. |
| 2. BBG Firmware Memory (Flash) 32 MByte | No | Yes | Firmware image for baseband generator | Firmware upgrade | | None required (no user data) |

Table 4-4 Vector Models with Baseband Generator (E4438C with Options 601 or 602)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|--|-----------------------------------|---------------------------------|--|---|---|----------------------------|
| 3. Coprocessor Memory (SRAM) 32 MByte | Yes | No | Operating memory of baseband coprocessor CPU | During normal operation, some user information, such as payload data, can remain in the memory. | This memory is used during normal baseband generator operation. It is not directly accessible by the user. Not battery backed. | Turn off instrument power. |
| 4. Buffer Memory (SRAM) 5 x 512 KByte | No | No | Support buffer memory for ARB and real-time applications | Normal user operation | This memory is used during normal baseband generator operation. It is not directly accessible by the user. Not battery backed. | Turn off instrument power. |

Table 4-5 Hard Disk (E4438C with Option 005)

| Memory Component, Type and Size | Writable During Normal Operation? | Data Retained When Powered Off? | Purpose/Contents | Data Input Method | Location in Instrument and Remarks | Sanitization Procedure |
|--|-----------------------------------|---------------------------------|---|---------------------------------|---|--|
| 1. Media Storage (Built-in Hard Disk) 6 GByte or 10 GByte (4 GByte usable in both cases) | Yes | Yes | User files, including flatness calibrations, IQ calibration, instrument states, waveforms (including header and marker data), modulation definitions, and sweep lists | User-saved data | The hard disk is an option for vector instruments (E4438C Option 005) and is therefore not installed in some instruments. If it is installed, these files are stored on the hard disk instead of in flash memory. | The magnetic residue requires several rewrite cycles or drive removal and destruction. User data is completely sanitized by the procedure “Erase and Sanitize All (Option 006 Only)” on page 22. |
| 2. Buffer Memory (DRAM) 512 KByte | No | No | Buffer (cache) memory | Normal operation, via hard disk | | Turn off instrument power. |

5 Memory Clearing, Sanitization and Removal Procedures

This chapter describes several security functions you can use to remove sensitive data stored in the instrument before moving it from a secure development environment. The functions described are:

- “Erase All (Option 006 Only)” on page 20
- “Erase and Overwrite All” on page 21
- “Erase and Sanitize All (Option 006 Only)” on page 22
- “Clear Persistent State Information” on page 23

CAUTION

These functions do **not** erase or sanitize external media connected to the instrument’s USB port.

CAUTION

Do not use the **Erase All**, **Erase and Overwrite All**, **Erase and Sanitize All**, **Erase, Overwrite**, or **Sanitize** procedure with any of these firmware revisions:

E44x8C: C.04.84, C.04.86, C.04.95

If your instrument’s current firmware revision is among those listed above, please upgrade **immediately** to newer firmware. For details, see “**Firmware Update Procedure**” on page 26.

Erase All (Option 006 Only)

This function removes all user files, user flatness calibrations, user I/Q calibrations, and resets all table editors with original factory values, ensuring that user data and configurations are not accessible or viewable. The instrument appears as if it is in its original factory state, however, the memory is not sanitized. This action is relatively quick, typically taking less than one minute (the exact time depends on the number of files).

| Model | Key Sequence |
|----------------|--|
| MXG (Series A) | File > More > Security > Erase All > Confirm Erase |
| ESG | Utility > Memory Catalog > More > Security > Erase All > Confirm Erase |

Note that there is a similar but distinct function, as described below, that deletes all user files but does **not** reset the table editors:

| Model | Key Sequence |
|----------------|--|
| MXG (Series A) | File > Delete All Files |
| ESG | Utility > Memory Catalog > More > Delete All Files |

Erase and Overwrite All

This function performs the same actions as **Erase All**, plus it clears and overwrites various memory types, as described below.

| Memory Type | Models | Description |
|---------------------------------------|---------------------|---|
| SRAM (Battery- backed) | Not MXG | All addressable locations are overwritten once with random characters. |
| CPU Flash | All | User data is erased with flash chip block-erase commands. No overwrite is performed. During erasure, the system files are temporarily moved to main memory and are then restored to CPU Flash when erasure is complete. |
| Extended Persistent Memory (Flash) | MXG N5162A/82A only | The file system is formatted, then all addressable locations are overwritten with random characters, and then the file system is reformatted again. |
| Hard Disk | ESG E4438C | All addressable locations are overwritten once with a random character. |

| Model | Key Sequence |
|----------------|--|
| MXG (Series A) | File > More > Security > Erase and Overwrite All > Confirm Overwrite |
| ESG | Utility > Memory Catalog > More > Security > Erase and Overwrite All > Confirm Overwrite |

Erase and Sanitize All (Option 006 Only)

This function performs the same actions as **Erase All**, plus it clears and overwrites the various memory types, as described below.

| Memory Type | Models | Description |
|---------------------------------------|---------------------|---|
| SRAM (Battery- backed) | PSG, ESG only | All addressable locations are overwritten once with random characters. |
| CPU Flash | MXG Series A ESG | User data is erased with flash chip block-erase commands. No overwrite is performed. During erasure, the system files are temporarily moved to main memory and are then restored to CPU Flash when erasure is complete. |
| Extended Persistent Memory (Flash) | MXG N5162A/82A only | The file system is formatted, then all addressable locations are overwritten with random characters, and then the file system is reformatted again. These actions are then repeated. |
| Hard Disk | ESG E4438C | All addressable locations are overwritten with a random character three times. |

| Model | Key Sequence |
|----------------|--|
| MXG (Series A) | File > More > Security > Erase and Sanitize All > Confirm Sanitize |
| ESG | Utility > Memory Catalog > More > Security > Erase and Sanitize All > Confirm Sanitize |

Clear Persistent State Information

The persistent state settings contain instrument setup information that can be toggled within predefined limits such as display intensity, contrast and the GPIB address. In vector models, the user IQ Cal is also saved in this area.

The following functions can be used to clear the IQ Cal file and to set the operating states that are not affected by an instrument power-on, preset, or *RST command to their factory default:

Instrument Setup

Key Sequence: MXG (Series A): **Utility > Power On/Preset > Restore System Settings to Default Values > Confirm Restore Sys Settings to Default Values**

ESG: **Utility > Power On/Preset > Restore System Defaults > Confirm Restore Sys Defaults**

SCPI Command: `:SYSTem:PRESet:PERSistent`

LAN Setup (MXG Only)

The LAN setup (hostname, IP address, subnet mask, and default gateway) information is not modified by an instrument power-on or *RST command.

MXG allows you to reset the instrument's LAN setup by using the following key sequence or SCPI command.

ESG does **not** offer this functionality.

Key Sequence: MXG (Series A) only: **Utility > I/O Config > LAN Setup > Advanced Settings > More 1 of 2 > Restore LAN Settings to Default Values > Confirm Restore LAN Settings to Default Values**

SCPI Command: MXG (Series A) only: `:SYSTem:COMMunicate:LAN:DEFaults`

User IQ Cal File (Vector Models Only)

When a user-defined IQ Calibration has been performed, the cal file data is removed by using the **Erase All (Option 006 Only)** feature, or by setting the cal file to default, as follows:

Key Sequence: **I/Q > I/Q Calibration > Revert to Default Cal Settings**

SCPI Command: MXG (Series A): `:CAL:IQ:DEF`

ESG: `:CAL:WBIQ:DEF`

6 Using Secure Mode

Secure Mode automatically applies the selected **Security Level** action the next time the instrument's power is cycled.

To activate Secure Mode, do the following:

| Step | Action | Notes |
|------|------------------------------|--|
| 1 | Open the Security Level menu | For MXG (Series A), press: File > More > Security > Security Level For ESG, press: Utility > Memory Catalog > More > Security > Security Level |
| 2 | Select the Security Level | Available options: <ul style="list-style-type: none"> – None – equivalent to a factory preset, no user information is lost – Erase – equivalent to Erase All (Option 006 Only) – Overwrite – equivalent to Erase and Overwrite All – Sanitize – equivalent to Erase and Sanitize All (Option 006 Only) |
| 3 | Activate Secure Mode | <div style="background-color: #FFD700; padding: 2px;">CAUTION</div> <p>Once you activate secure mode (by pressing Confirm), you cannot deactivate or decrease the Security Level; the erasure actions for the selected Security Level execute at the next power cycle. Once you activate Secure Mode, you can only increase the Security Level until you cycle power. For example, you can change Erase to Overwrite, but not the reverse.</p> <p>After the power cycle, the Security Level selection remains the same, but the secure mode is not activated.</p> <p>For MXG (Series A), press: File > More > Security > Enter Secure Mode > Confirm</p> <p>For ESG, press: Utility > Memory Catalog > More > Security > Enter Secure Mode > Confirm</p> <p>The Enter Secure Mode softkey changes to Secure Mode Activated.</p> |


7 Using Secure Display

This function prevents unauthorized personnel from reading the instrument display or tampering with the current configuration via the front panel. When Secure Display is active, the display is blank, except for an advisory message, as shown in [Figure 7-1](#) below. All front panel keys are disabled.

To set Secure Display, press: **Utility > Display > More > Activate Secure Display > Confirm Secure Display**

Once Secure Display has been activated, the power must be cycled to re-enable the display and front panel keys.

Figure 7-1 Signal Generator Screen with Secure Display Activated

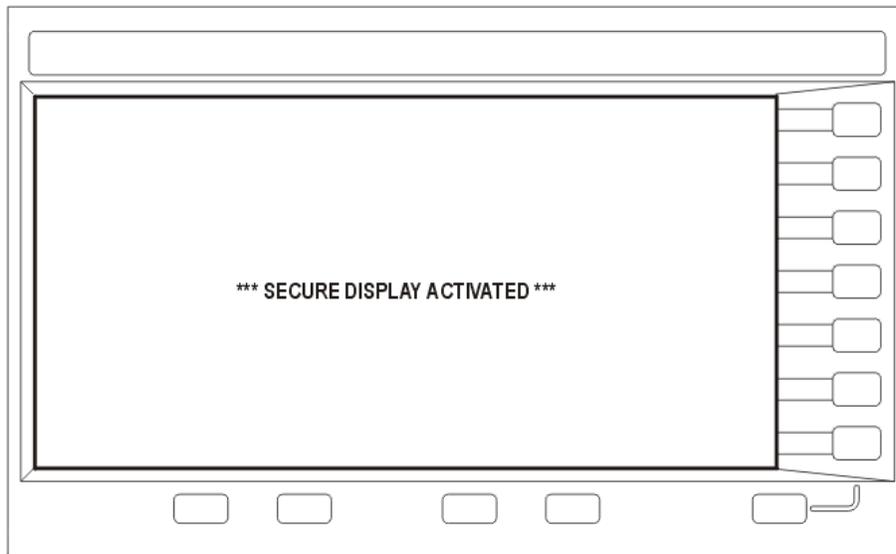

8 Security Issues for Certain Firmware Revisions

If your instrument currently has one of the firmware revisions listed in [Table 8-1](#), using certain security features may cause the deletion of some of the instrument's system files. Before using the security features, update your firmware to the appropriate revision listed in the "Update to" column of [Table 8-1](#).

Table 8-1 Firmware Revisions by Instrument Model

| Model | Affected firmware revisions | Update to |
|--------|------------------------------|------------------|
| E4428C | C.04.84, C.04.86, or C.04.95 | C.04.96 or later |
| E4438C | C.04.84, C.04.86, or C.04.95 | C.04.96 or later |

Firmware Update Procedure

To obtain the latest firmware online, perform the following steps:

- 1. Access the instrument's web page:**
www.keysight.com/find/<model_number> (Example:
www.keysight.com/find/E4438C).
- 2. Under the **Technical Support Tab**, select **Drivers and Software**, and follow the remaining links to the firmware upgrade page.**

If web access is not available, Keysight can provide the new firmware on CD-ROM. To obtain the CD-ROM, contact Keysight or your Keysight representative, as described in ["Contacting Keysight Sales and Service Offices"](#) on [page 5](#).

Error Messages and Secure Environments

If you cannot upgrade the firmware prior to using the security features, Keysight will help you to recover from error messages that may appear after executing the security functions. The error messages indicate that instrument system files have been erased. The following list shows some possible error messages:

- 256, File name not found; /SYS/LICENSE.TXT
- 617, Configuration Error; License file not found. Creating empty one.
- A missing or damaged system file was encountered while trying to diagnose the system.

Even if these error messages appear, the security function has completely sanitized the instrument. If the instrument is located in a secure environment, it is safe to remove it. After removing it from the secure area, follow the process below to recover the lost system files.

Recovering Erased System Files

To recover the lost files, perform the following steps:

1. Obtain your instrument's model and serial number.
2. Contact Keysight and request a replacement license file.
The Keysight representative will ask for the model and serial number.
3. Update the firmware to the revision specified in the "Update to" column of [Table 8-1 on page 26](#).
 - a. If problems occur when upgrading the firmware, manually enter as many license keys as possible using **Utility > Instrument Adjustments > Instrument Options > Software Options**
 - b. Upgrade the firmware again.
4. Open Internet Explorer and enter `http://<instrument IP address>/update`.
5. Locate **Recover Self-test System Files** and click **Execute**.
6. Locate **Overwrite LICENSE.TXT**, cut and paste the replacement license file (obtained in Step 2) into the text box, and click **Execute**.
7. Cycle the power on the instrument.
8. If configuration errors persist after completing the previous steps, contact Keysight again.

9 Procedure for Declassifying a Faulty Instrument

If the instrument is not functional, and you are unable to use the security functions, you may physically remove the Processor board and Hard Disk or Solid State Drive (if installed).

For removal and replacement procedures, refer to the [Service Guide](#) for your instrument.

Once the Processor and Hard Disk assemblies have been removed, proceed as in [Table 9-1](#) below:

Table 9-1 Assembly Disposal Procedures

| Assembly | Procedure |
|------------------------------------|---|
| Processor (CPU) Board | <p>Either</p> <p>Discard the processor board and send the instrument to a repair facility. A new Processor Board will be installed, then the instrument will be repaired and calibrated. If the instrument is still under warranty, you will not be charged for the new Processor Board.</p> <p>or</p> <p>If you have another working instrument, install the Processor Board into that instrument and erase the memory. Then reinstall the Processor Board back into the non-working instrument and send it to a repair facility for repair and calibration. If you discover that the Processor Board does not function in the working instrument, discard the Processor Board and note that it caused the instrument failure on the repair order. If the instrument is still under warranty, you will not be charged for the new Processor Board.</p> |
| Hard Disk (E4438C Option 005 only) | <p>Either</p> <p>Discard the Hard Disk and send the instrument to a repair facility. Indicate on the repair order that the Hard Disk was removed and must be replaced. A new Hard Disk will be installed, then the instrument will be repaired and calibrated. If the instrument is still under warranty, you will not be charged for the new hard disk.</p> <p>or</p> <p>Keep the Hard Disk and send the instrument to a repair facility. When the instrument is returned, reinstall the Hard Disk.</p> |

A: References

1. **DoD 5220.22-M, “National Industrial Security Program Operating Manual (NISPOM)”**
United States Department of Defense. Revised February 28, 2006.
http://www.dss.mil/isp/fac_clear/download_nispom.html
2. **ISFO Process Manual for the Certification and Accreditation of Classified Systems under the NISPOM**
Defense Security Service.
DSS-cleared industries may request a copy of this document via email, by following the instructions at:
<http://www.dss.mil/isp/odaa/request.html>
3. **Greenliant NANDrive Security Erase Feature, Purge Command Specification**
This Application Note may be obtained in PDF format from Greenliant Systems Ltd., by contacting the company via their web site:
http://www.greenliant.com/contact_us
4. **ATA Attachment 8 - ATA/ATAPI Command Set (ATA8-ACS)**
INCITS Technical Committee T13/1699-D Revision 6a, September 6th, 2008
This standard may be downloaded in Acrobat (PDF) format from the INCITS T13 web site:
<http://www.t13.org/documents/UploadedDocuments/docs2008/D1699r6a-ATA8-ACS.pdf>
5. **Installation Guide**
Keysight Technologies Inc. Specific to Signal Generator model
MXG (Series A): <http://literature.cdn.keysight.com/litweb/pdf/N5180-90002.pdf>
ESG: <http://literature.cdn.keysight.com/litweb/pdf/E4400-90502.pdf>
6. **Programming Guide**
Keysight Technologies Inc.
<http://literature.cdn.keysight.com/litweb/pdf/N5180-90005.pdf>
7. **SCPI Programmers Reference**
Keysight Technologies Inc. Specific to Signal Generator model:
MXG (Series A): <http://literature.cdn.keysight.com/litweb/pdf/N5180-90004.pdf>
ESG: <http://literature.cdn.keysight.com/litweb/pdf/E4400-90506.pdf>

References

8.

Service Guide

Keysight Technologies Inc.

N5161A/62A/81A/82A/83A MXG (Series A) Signal Generators

<http://literature.cdn.keysight.com/litweb/pdf/N5180-90006.pdf>

E4428C/38C ESG Signal Generators

<http://literature.cdn.keysight.com/litweb/pdf/E4400-90511.pdf>



This information is subject to change without notice.

© Keysight Technologies 2004-2017

Edition 3, October 2017

E4400-90621

www.keysight.com